


ORNL



NEUTRON SCIENCES




**Thermo Scientific
NanoDrop 1000
Spectrophotometer**

4 Cleaning Guide


Sample Forms
Liquid Column
Here

2

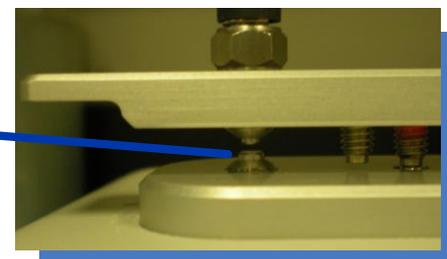

Sample
Arm


3

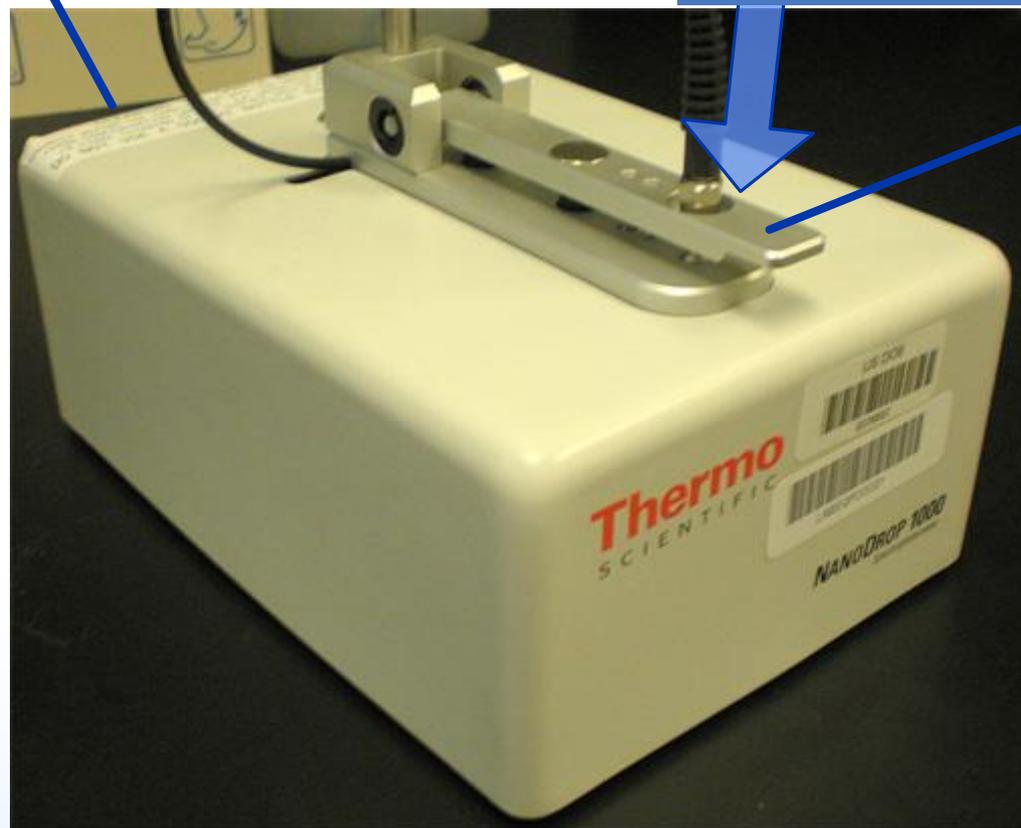


1

Icon to Launch
Operating
Software

SETUP

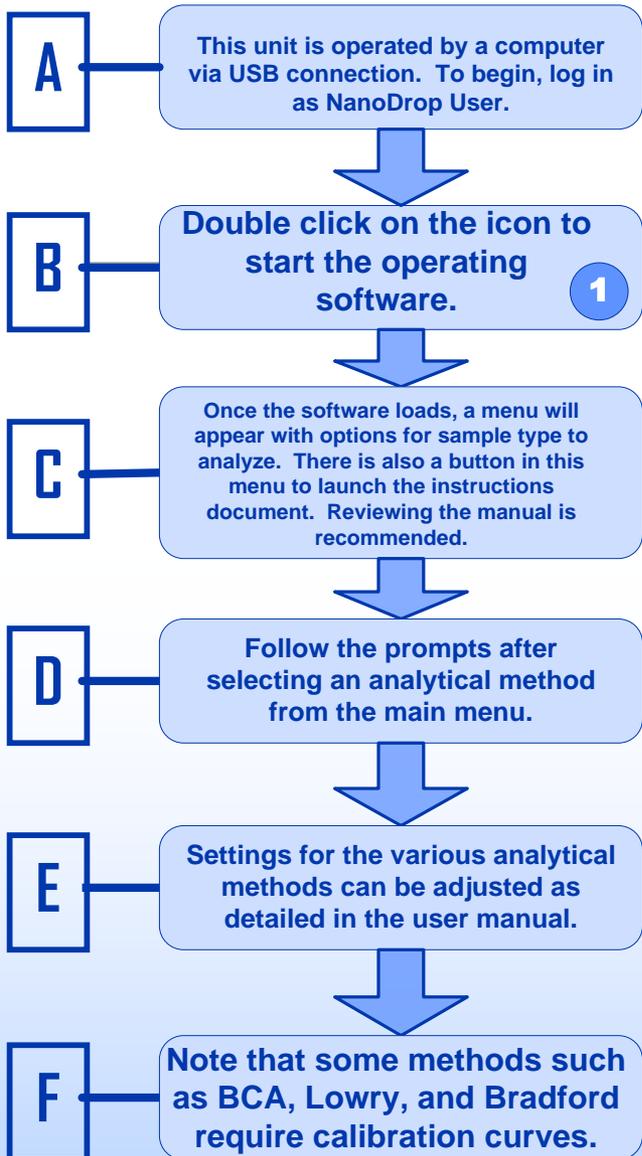

OPERATION

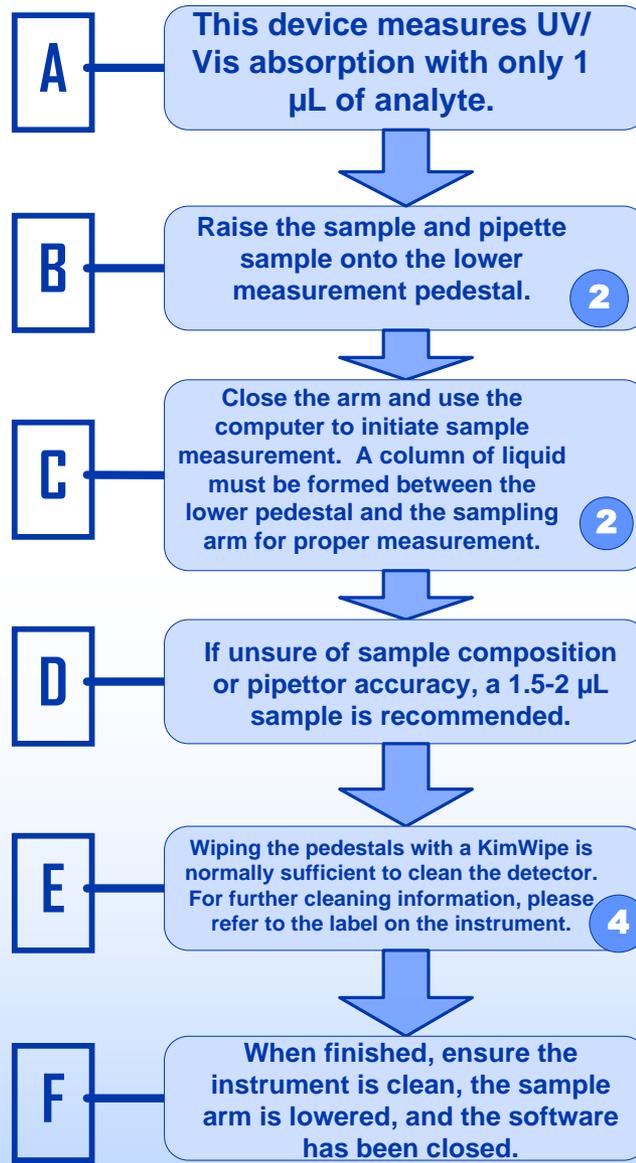

HAZARDS



ELECTRICAL HAZARD

This equipment contains liquid near electrical connections.



TOXIC HAZARD

Some protein assay reagents are harmful on exposure to tissues.

PREVENTION



EYE PROTECTION

Wear safety glasses while operating.



PROTECTIVE GLOVES

Wear appropriate gloves for heat and chemical usage.



NON-SLIP, CLOSED SHOES

Wear non-slip, closed shoes to avoid spills.



READ MANUAL

Become familiar with this guide before operating.

For additional help contact the Lab Space Manager