




VWR Orbital Shaking Incubator  
Model: 1575R

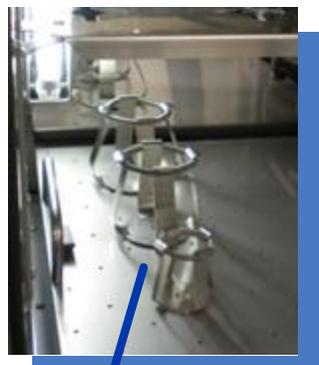


7 Bottom Shelf with Attachment Points for Sample Holders

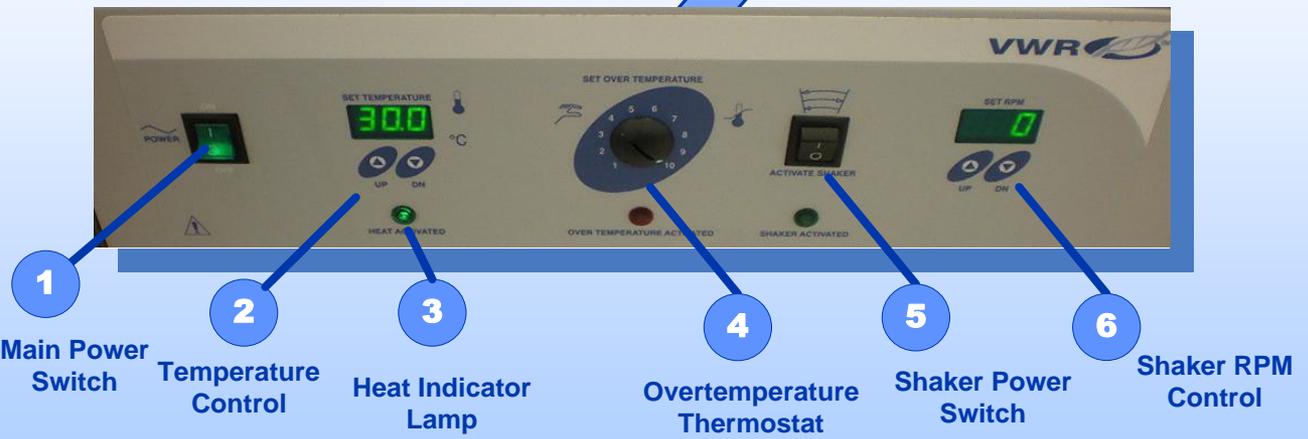

# SETUP

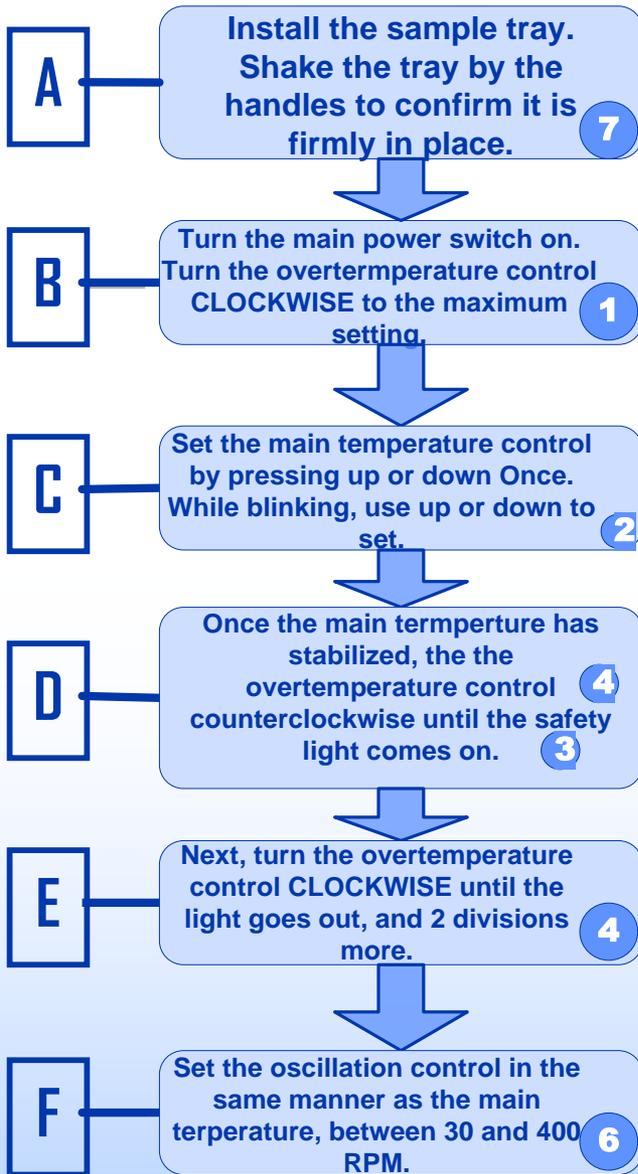

# OPERATION

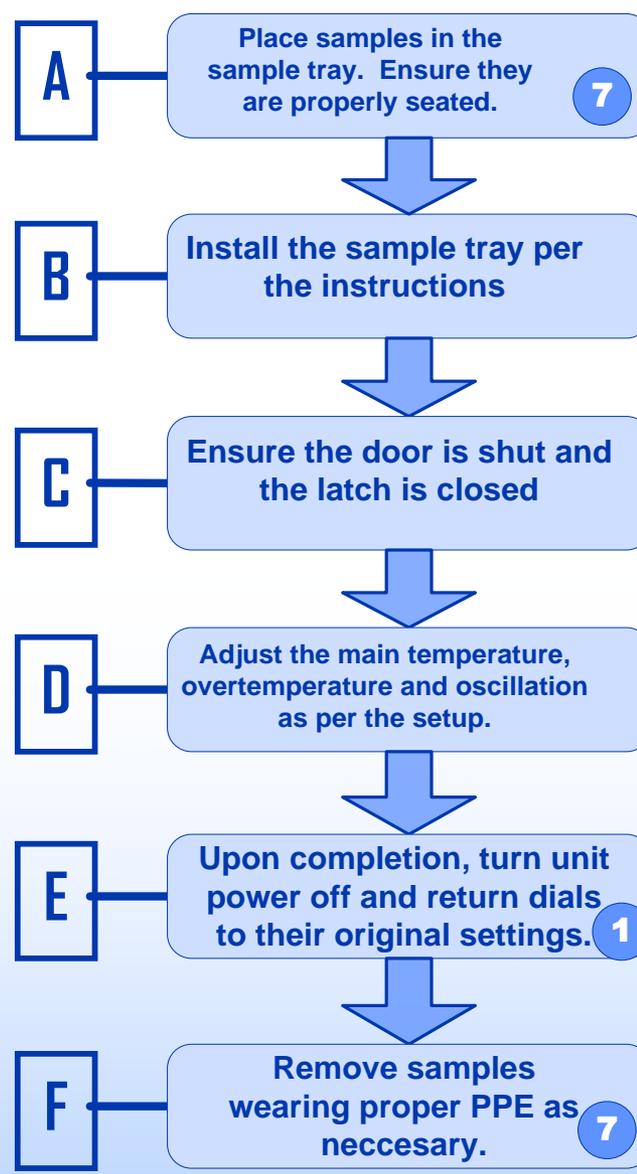

# HAZARDS



## ELECTRICAL HAZARD

This equipment contains liquid near electrical connections.



## HEAT HAZARD

This equipment produces heat may cause burns.



## PINCH HAZARD

This equipment has a door and moving parts within the cabinet that may pinch body parts or clothing.



## Chemical Hazard

Because chemicals are being placed in this unit, chemical hazards are present.



## Fire Hazard

Improper use of this unit may cause a fire hazard.

# PREVENTION



## EYE PROTECTION

Wear safety glasses while operating.



## PROTECTIVE GLOVES

Wear appropriate gloves for heat and chemical usage.



## NON-SLIP, CLOSED SHOES

Wear non-slip, closed shoes to avoid spills.



## READ MANUAL

Become familiar with this guide before operating.

For additional help contact the Lab Space Manager